



# TIDE Mass\_3

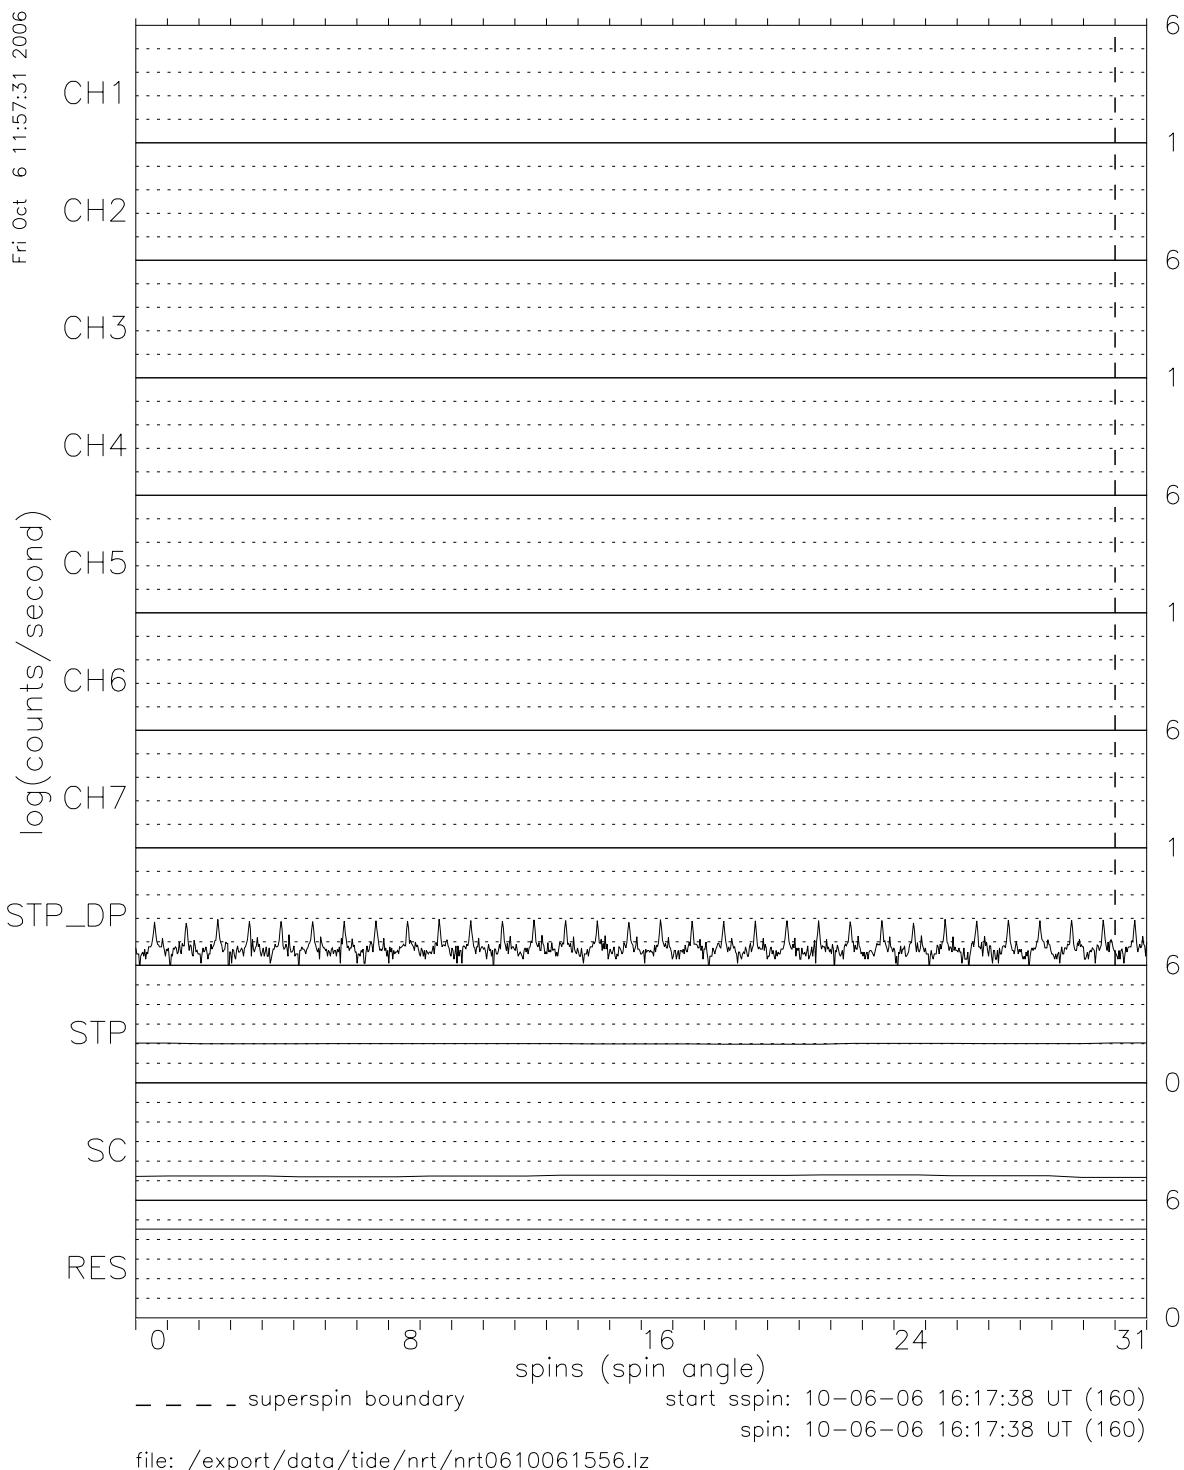

-15kV TOF: -9181 v  
 -3.6kV MCP: -3379 v  
 -2.4kV MCP: -1784 v  
 Input Cur: 310 ma  
 RPA max: 237 v  
 Mirror max: 238 v

Fri Oct 6 11:57:32 2006

## TIDE Direct Events

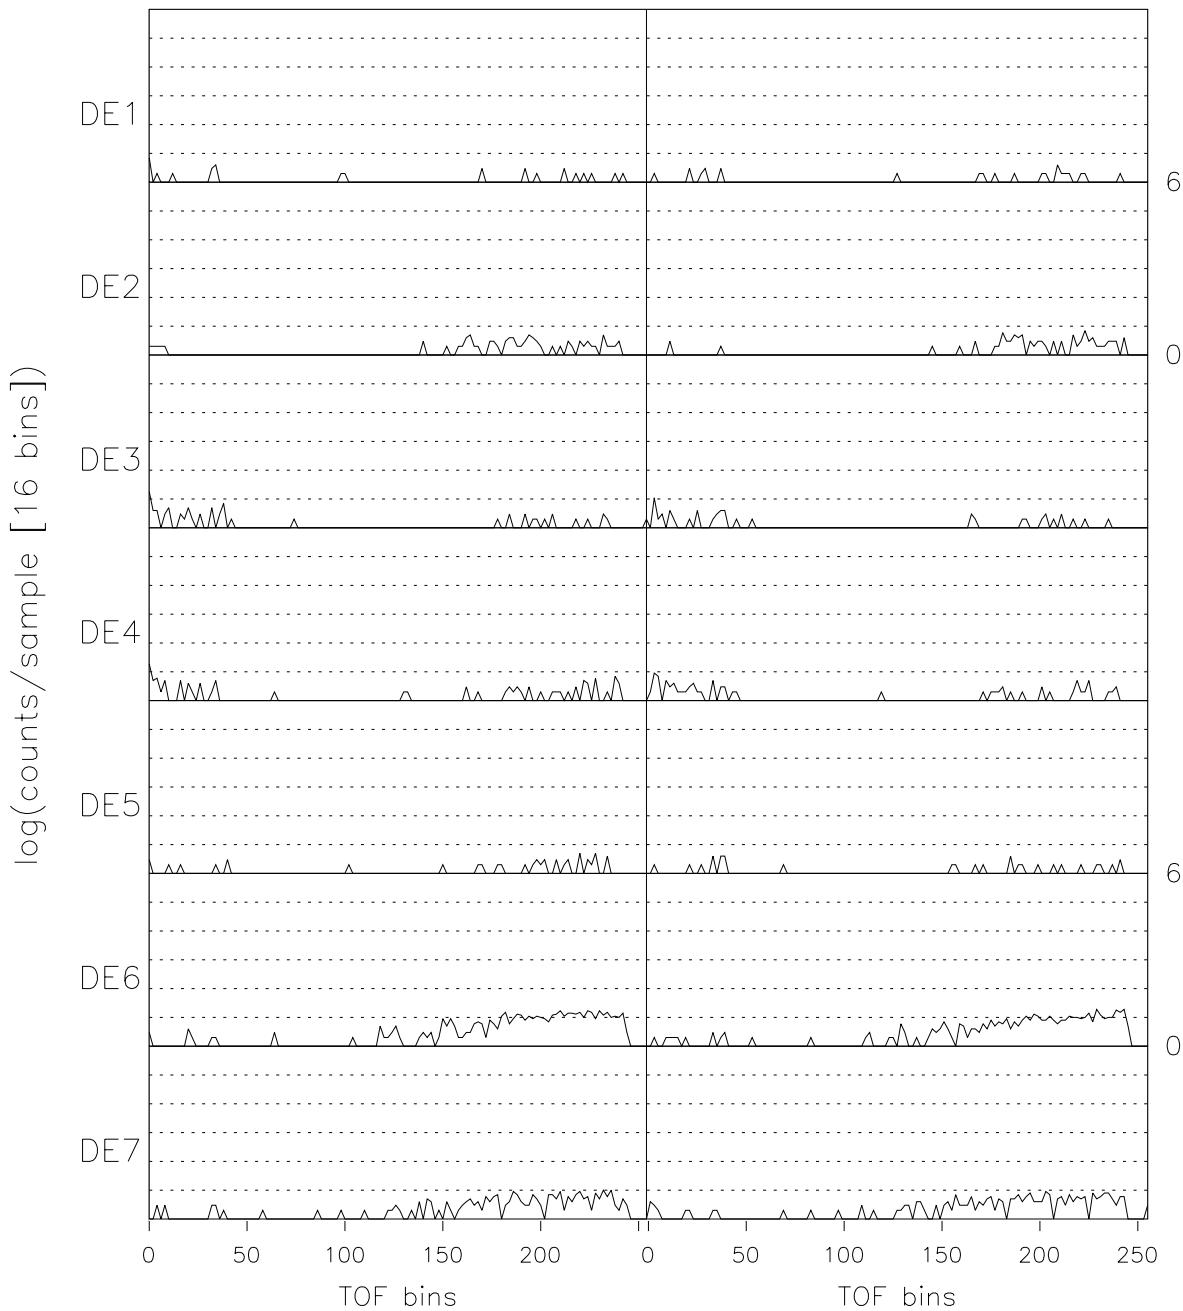

reported: 10-06-06 16:11:07 UT

reported: 10-06-06 16:14:20 UT

file: /export/data/tide/nrt/nrt0610061556.lz

-15kV TOF: -9181 v  
-3.6kV MCP: -3379 v  
-2.4kV MCP: -1774 v  
Input Cur: 312 ma  
RPA max: 237 v  
Mirror max: 238 v